Carestream Health Mammography Processing Control Chart

Processor Film Emulsion Number Year

Date Crossover Performed _____ Crossover Emulsion Number _____



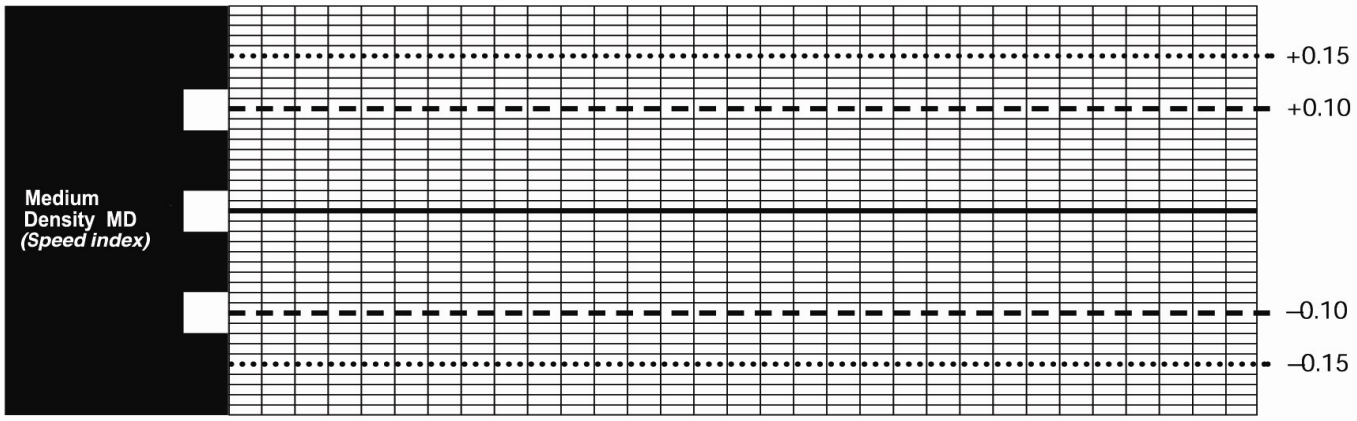

Step # _____

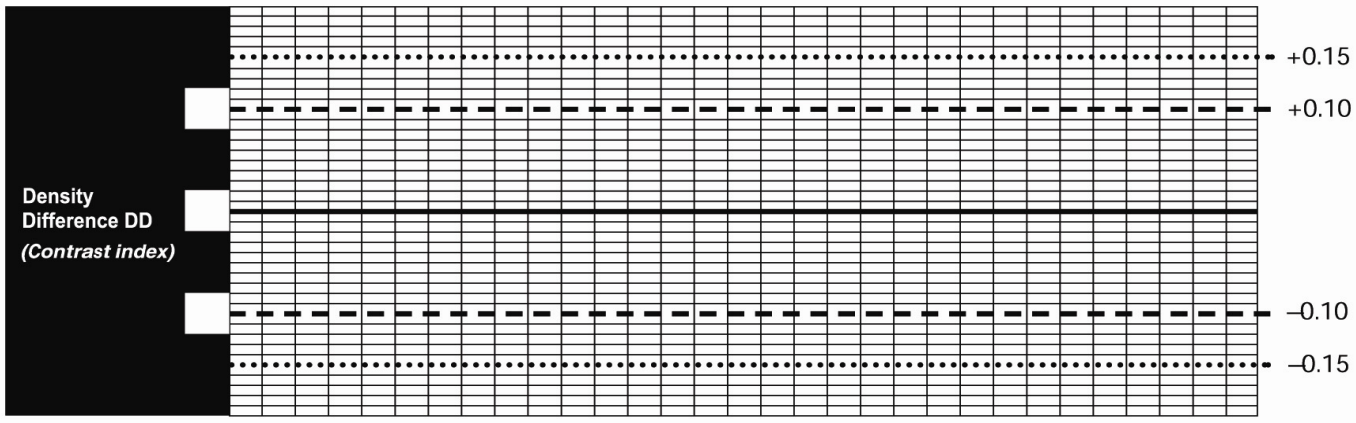

Step # _____ Step # _____



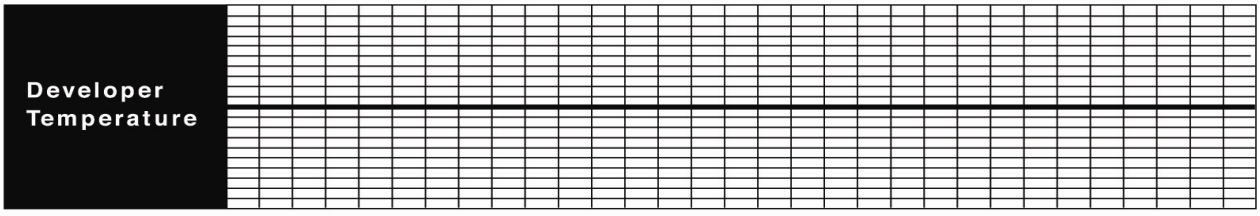

Replenishment Rates per
number of films _____
film size _____
length of film travel _____

Date	Developer	Fixer

Carestream

Record remarks on the back of this sheet.

Carestream Health Mammography Processing Control Chart

Date	Action	Date	Action

M7-173 Printed in U.S.A. © Carestream Health, Inc., 2007

Carestream